# The History of Quadrupole Mass Spectrometry at VG - Micromass - Waters

Mike Morris, Steve Bajic, Kate Whyatt, Keith Worrall, Dave Gordon, Mark Roberts, Richard Moulds, Lance Nicolaysen, Nicholas Ellor, Viki Brooks, Amir Faroog

### **COMPANY BACKGROUND**

VG Instruments was formed in 1962 (Vacuum Generators Limited) to provide ultra-high vacuum components and systems. In 1970, VG Micromass<sup>™</sup> was formed to specialise in mass spectrometry and in 1974 was fragmented into four: VG Isotopes, VG Organic, VG Quadrupoles and VG Inorganic. VG Organic moved to Altrincham, South Manchester, UK, along with VG Data Systems. The rationale behind the repeated formation of small companies was


Bernard Eastwell's 'Christmas card principle' : most people send Christmas cards to between 50 and 100 people. and this represents a natural maximum number of people with whom to associate in a company. In 1980, VG Analytical was formed, followed by VG Masslab (1984), VG Tritech (1985) and VG Biotech (1988).



VG Altrincham Facility c.2000

### SINGLE QUADRUPOLES

The first quadrupole mass filters from the VG stable were introduced in 1971 by VG Quadrupoles, with the Q7 (m/z range 120) and the Q8 (m/z range 300), and were made available in either kit form or as complete analytical systems. Both the Q7 and Q8 used 6mm guadrupole rods for residual gas analysis (RGA) applications. These instruments were followed by the Q40 and Q50 devices that used 12mm and

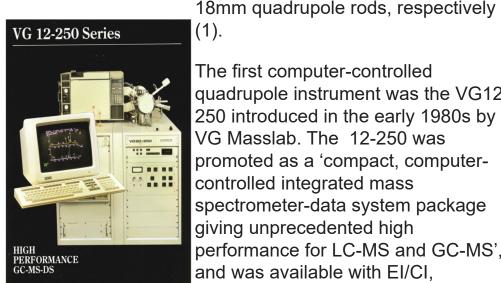

he first computer-controlled uadrupole instrument was the VG12-250 introduced in the early 1980s by /G Masslab. The 12-250 was promoted as a 'compact, computercontrolled integrated mass spectrometer-data system package

giving unprecedented high performance for LC-MS and GC-MS', and was available with EI/CI,

Thermospray, moving belt LC-MS and VG 12-250 Fast Atom Bombardment ion sources. The data system was a PDP11-73 with a massive 70MB system storage and a 90MB streaming tape.

In 1985, VG MassLab introduced the benchtop GC/MS TRIO-1 instrument with a m/z range of 1000, and incorporated the

same quadrupole assembly as was used across all the quadrupole range. It had the capability of using direct-inlet capillary GC columns, as well as the facility for using packed GC columns with a jet



TRIO 1

The second generation of the TRIO-1 in 1988, the TRIO 1000, saw the introduction of the PC-based data system and LabBase instrument control and data processing. The TRIO-2 was a research-targeted multi-inlet (GC/LC-MS) single guadrupole instrument with an increased mass range vs the TRIO-



TRIO 2

In 1993 VG Biotech introduced the multi-inlet Platform single quadrupole, a compact benchtop instrument intended as a detector for the chromatographer's bench. This was the first



time that external design consultants were used by VG in the development of an instrument. Electrospray capabilities were updated to accommodate LC flow rates of up to 1.0mL/ min that served to

VG Platform

interface with 4.6mm HPLC

columns. This was the first instrument to be launched with the Windows-based MassLynx<sup>™</sup>

data system. Other capabilities that were introduced with the Platform series included Open Access analysis for synthetic chemists, and the MaxEnt deconvolution software for use in the analysis of proteins. There were also a number of these instruments that were modified to deliver



ZMD 2000 accurate mass measurement (<5ppm to m/z 500) in a routine environment using 18-bit Digital to Analog converters(2).

In 2000, a pair of instruments based on the same architecture was released - the Waters<sup>™</sup> ZQ single quadrupole and the

instruments

designed to



to be part of an LC-MS system. The integration with liquid chromatography was taken a step further in 2005 with the delivery of the single and tandem quadrupole

Quattro micro triple guadrupole. Both


of these instruments were designed

ZQ 2000

work with the ACQUITY UPLC<sup>™</sup> system, cunningly entitled the SQD and TQD, facilitating method development with the introduction of on-board fluidics and new software functionality.



ACQUITY SQD

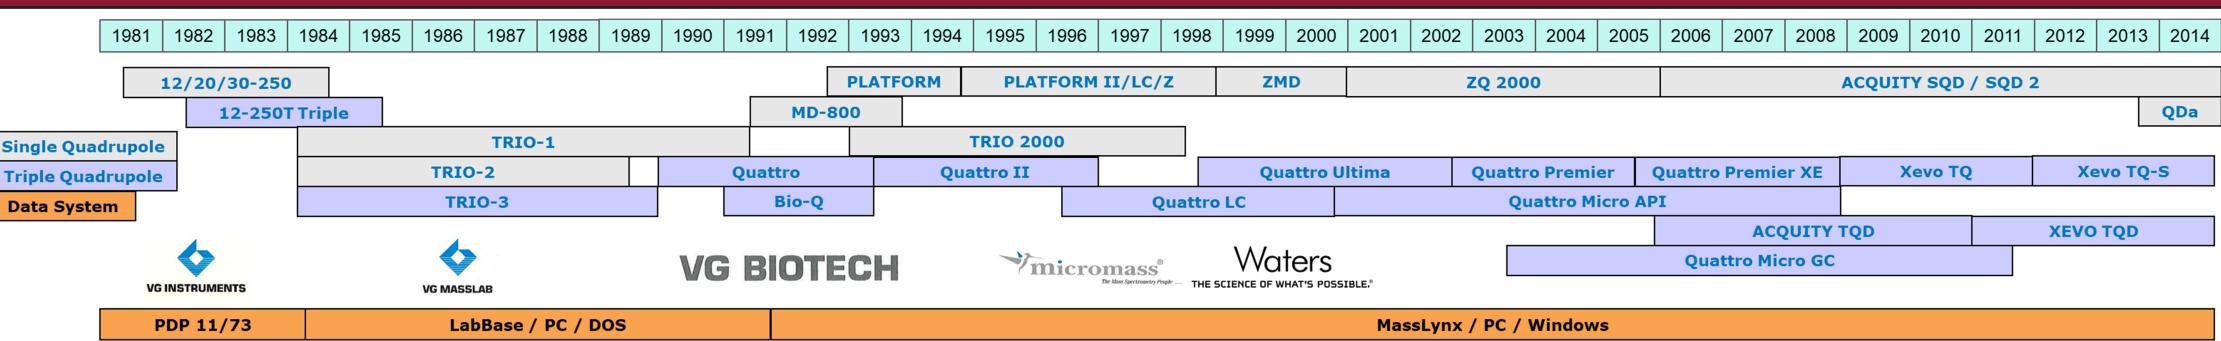

The current state-of-the-art single quadrupole, the QDa<sup>™</sup>. was launched in late 2013, and specifically designed as a detector for use with liquid chromatography. The QDa was the first mass detector fully configured within an LC stack,



with the intention of bringing the benefits of mass spectrometry to the chromatographer, and incorporated built-in calibration and operation with broad tuning parameters

### TANDEM QUADRUPOLES

The first triple quadrupole instrument from VG Masslab in



984 was the TRIO 3 with dual optical detectors and controlled with a PDP11/73 data system. The dual detectors permitted switching between MS and MS/MS modes in 50ms, and allowed mixed mode scanning experiments as well as

TRIO 3 data-dependent analyses.

The first, dedicated atmospheric pressure ionisation triple quadrupole was introduced in 1991 as the VG Bio-Q, with electrospray ionisation. The Bio-Q was marketed primarily for


infusion analysis of proteins, in combination with MaxEnt deconvolution. This instrument was also the last quadrupole system that used diffusion vacuum pumps.

The Bio-Q was followed in 1992 by the multi ion source Quattro I with m/z 4,000 guadrupoles and two detectors.



Bio Q

In 1994, the Quattro I was followed by the Quattro II which

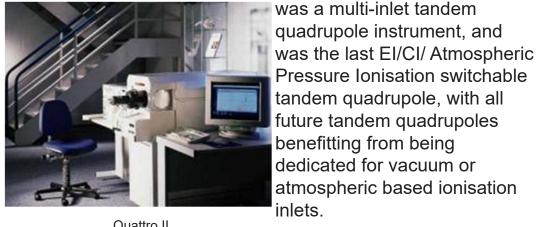

The first benchtop triple quadrupole was the Quattro LC, introduced in 1996, which had mass range options of m/z 1,600 and m/z 4,000 depending on the target applications. This was the first Micromass instrument to use RF-transfer lenses between the ion source and the analyser. The Quattro LC also saw a move

away from the embedded transputer control system to embedded PC control, as well as the introduction of the dualorthogonal Z-spray API ion source, internally referred to as the

'goldfish bowl'. The introduction of the

multiplex (MUX) interface in 1999 allowed for the introduction of 4 or 8 parallel LC streams simultaneously into the ESI source.

The drive for the highest possible levels of instrument



sensitivity led to the exploration of multiple stages of differential pumping in the transport region between the ion source and the mass analyser. The Quattro Ultima was introduced in 2000, with two stages of differential

pumping, and a revised detector Quattro Ultima Pt with greater gain. This was superseded by the Quattro Ultima Platinum in 2002, which included for the first time, RF ion tunnels in place of the hexapole RF ion guides.



uture tandem quadrupoles

atmospheric based ionisation

Quattro LC


smallest tandem increase lab metabolic screening.



residence time of the ions in the collision cells. This was addressed in the Quattro Premier with the introduction of a travelling wave (T-Wave) RF device as the collision cell between the two massanalysing quadrupoles.

The ACQUITY<sup>™</sup> SQD/TQD systems were the first quadrupole instruments designed to cope with UPLC



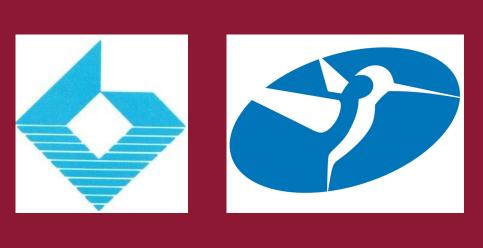

## Waters THE SCIENCE OF WHAT'S POSSIBLE.

ZMD ZQ 2000 ACQUITY SQD / SQD 2 QDa **Quattro Premier XE Quattro Premier** Xevo TQ Xevo TQ-S **Quattro Ultima Quattro Micro API ACQUITY TQD XEVO TQD** Waters Quattro Micro GC THE SCIENCE OF WHAT'S POSSIBLE. MassLynx / PC / Windows

When it was introduced in 2001, the Quattro micro was the

quadrupole instrument commercially available. This instrument was a start in addressing the increasing cost of laboratory bench space and the need to productivity. The Quattro micro was the first MS/MS instrument available for *in vitro* 



Quattro micro diagnostic (IVD) applications, with an initial focus on neonatal

With the adoption of faster

quantify higher numbers of

compounds to increase

chromatography and the need to

laboratory throughput, the speed

of multiple reaction monitoring

(MRM) analysis became limited

In 2003, the Quattro micro GC was introduced, with direct probe EI/CI capabilities alongside a GC interface.

by the





Xevo TQD

**Quattro Premier** separations in 2005. The next iteration, the Xevo<sup>TM</sup> TQD in 2010, included the addition of the universal ion source architecture, stacked-ring ion guides in the source transfer optics, and new electronics to permit faster scanning.

The Xevo TQ was introduced in 2008 as a high-performance instrument and brought the time-saving and consistency of automated acquisition and processing method creation to market, along with the capability to perform GC/MS on an atmospheric pressure ionisation mass spectrometer with the APGC interface. The Xevo TQ also saw enhancements in



usability with the introduction of the Universal Ion Source that would allow for a full range of ionisation techniques to be used by fitting the relevant from ESI/APcI/EScI, APGC<sup>™</sup>, APPI, ASAP™, nano-ESI or TRIZAIC<sup>TM</sup> probe. The Xevo TQ also contained the T-Wave collision cell, and some new modes of operation were introduced with the ability to trap and release ions in synchronisation with the scanning of the second

quadrupole mass filter.

Xevo TQ

In 2010, a breakthrough in ion optical design was made with the introduction of the StepWave<sup>™</sup> ion guide, specifically designed to capture as much of the ion beam as possible

from the atmospheric pressure region after entry into the high vacuum system of the mass spectrometer. The dual ion tunnel design of the Stepwave ion guide enabled the efficient extraction of ions from the primary plume entering the vacuum region, and the rejection of unwanted particles/neutrals.



Xevo TQ-S

### **REFERENCES:**

(1) R H Bateman in K R Jennings (Ed.) A History of European Mass Spectrometry, IM Publications, (2012). (2) A N Tyler, E Clayton and B N Green, Anal.Chem. 68 (1996) 3561.

Waters, Micromass, MassLynx, ACQUITY, ACQUITY UPLC, QDa, Xevo, APGC, ASAP, TRIZAIC and StepWave are trademarks of Waters Technologies Corporation.